

HORIBA

LAQUAtwin

Waterproof Pocket Water Quality Meters



Agriculture



Aquaculture



Arts



Food &
Beverage



Health
Management



Livestock



Manufacturing



Water &
Wastewater




www.horiba-laqua.com

MADE IN
JAPAN

Explore the future

HORIBA

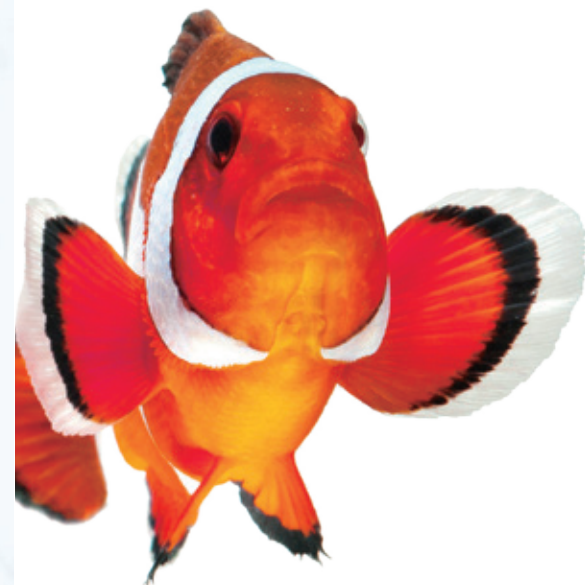

Contents

Product Overview	4
Product Features	6
Applications	9
Meter Specifications	14
LAQUAtwin pH Meters	15
LAQUAtwin ORP Meter	15
LAQUAtwin Conductivity / TDS Meters	16
LAQUAtwin Salinity Meter	16
LAQUAtwin Ion Meters	17
Accessories & Solutions	18



LAQUA[®]twin



Pocket Water Quality Meters

Lab in your pocket.

Maximise On-the-Go Testing with Expanded Water Quality Parameters — Now 10



Quick & Simple

- Measure directly – no container required
- Only a few drops of sample needed



Battery & Safety Features

- Powered by 2 x CR2032 batteries
- Secure battery cover to prevent accidental opening



Unique Flat Sensor Design

- Requires as little as 50µL with sampling sheet
- Multiple measurement techniques



Reliable and Proven Technology

- Backed by over 70 years of HORIBA expertise
- Uses miniaturized components identical to lab instruments



User-Friendly Operation

- Clear backlit display with ☺ indicator for stable readings
- Convenient single-button calibration / measurement



Cost Effective

- Uses only 1/100th of the standard / sample volume
- Features replaceable sensors to extend meter's lifespan



Portable & Built for On-Site Testing

- Get immediate, reliable results in the field
- IP67 dustproof and waterproof for rugged environments
- Comes with protective carrying case

Scan For
Introduction
Video



Easy Measurement for All Users

Measurement Button

Press to view mV or temperature (Auto Stable mode) or to lock / unlock reading (Auto Hold mode).

In Set-up mode, press to scroll or adjust settings.

Meter

Rated IP67 waterproof and dustproof

Sensor

Rated IP67 waterproof and dustproof.

Sensor is easily replaceable.



Scan For
How to Insert
Sensor/Battery
Video



Scan For
Calibration
Video



Scan For
Measurement
Video



Strap Hole

You can attach a strap or tag here.

Power Button

Press to switch on or off the meter or exit set-up mode.

Calibration Button

Press to perform calibration or save settings in set-up mode.

Backlight

For easy viewing in the dark. Flashes when battery is low.

Sensor Guard

Protects sensor from damage and light. Sliding cap—for scooping water samples. Open the whole sensor guard when placing water or solid samples directly onto the sensor.

Slide Cap



1 Battery Indicator

Appears when battery is low

2 Calibration Mark

Calibration is complete when it stops flashing.

3 Measurement Mark

Measurement is complete when it stops flashing.

4 Measurement Value

Flashes when the measurement value is out of the range.

5 Stability Mark

Lights up when measurement is complete.

6 Temperature Alarm

It flashes when the temperature is out of range.

7 Voltage Measurement Mode

Displays sensor voltage

IMMERSION

When you're in the lab, you can test the sample in a beaker. Ensure the sensor guard sliding cap is open.



SCOOP

Use as a scoop to test water from a river. Vertical scoop is available with a unique sensor guard.



DROPS

Drop a sample with a dropper; volumes as small as 0.1 mL can be measured. By using sampling sheet B, volumes down to 0.05 mL can be tested.



UNIQUE MEASUREMENT OPTIONS

One meter provides seven flexible measurement techniques. Simply choose the method that best fits your sample and situation.

WIPE

The sampling sheet enables tiny, trace volume analysis. For example, wiping the skin with a water-soaked sampling sheet and measure.




SOLID SAMPLES

Foods containing some moisture can be tested by placing a small piece directly onto the sensor.



POWDERS

LAQUAtwin meters can also test dry powders. Simply place the powder sample onto the sensor, and add an appropriate amount of pure water.



PAPER, TEXTILES AND FILMS

To test sheets of paper and textiles, cut the sample into small pieces, place directly on the sensor, and add a defined amount of pure water.



*All methods applicable to pH measurement. Conductivity models cannot be tested with solids, powders, and sheet-like samples. Above pictures are for illustration purposes only.


10 Water Quality Parameters

Using the same measurement principles as laboratory instruments, LAQUAtwin pocket meters deliver reliable, accurate water quality results. Choose the ideal meter for your application from 13 vibrant, easy to use models.




Hassle-Free Operation

Calibrate and measure at the touch of a button. A smiley face icon appears to confirm a stable reading.

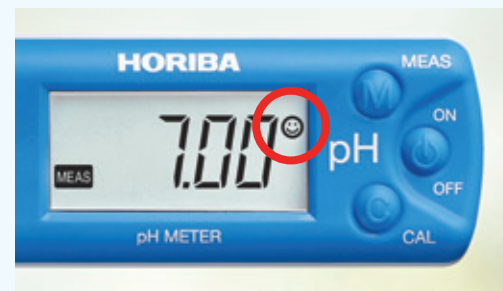

Advanced Sensor Technology

LAQUAtwin sensors are engineered with the same technology as standard laboratory electrodes, miniaturized into an ultra thin flat sensor—less than 1 mm thick—and backed by over 70 years of HORIBA sensor expertise.

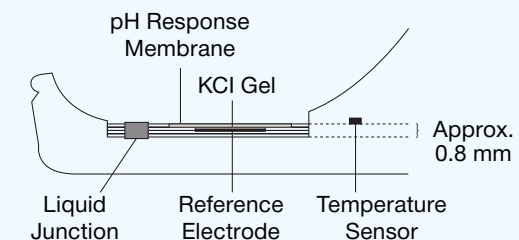

Cross-sectional view of the flat pH sensor chip

Rated IP67 Waterproof & Dustproof¹

Built for testing anywhere, anytime, the LAQUAtwin's IP67 rating protects the meter against dust and water exposure—perfect for fieldwork, outdoor sampling, and unpredictable conditions.



¹ Withstand immersion for 30 minutes at 1m depth. Not suitable for underwater use.

Bright Backlit Display

The backlit screen ensures clear readings even in low light environments and shows a stability indicator, with an option to freeze the value automatically in Auto Hold mode.



Complete Testing Kit

All essential accessories are stored in a compact carrying case, with the option to attach your own strap or tag for added convenience during on the go measurements.



Applications



pH AND CONDUCTIVITY MEASUREMENTS IN COCONUT COIR SUBSTRATE



Coconut coir testing involves extracting a sample solution with distilled water and measuring the pH and conductivity of the extract. The acceptable conductivity ranges for 1:2 (v/v) dilution and pour thru sampling methods are 0.26-0.75 mS/cm and 1.0-2.6 mS/cm, respectively. The ideal pH range is 5.4-6.2 for both methods.



SCAN QR CODE FOR LINK



DETERMINATION OF NUTRIENT CONCENTRATIONS IN SOIL SOLUTION AND TOMATO PLANT SAP



Fertigation management requires rapid and accurate methods to determine nutrient concentrations in soil solution and plant sap. Folegatti et al (2005) concluded that LAQUAtwin meters are useful low-cost tools in fertigation management as their measurements of NO₃⁻, K⁺, and Na⁺ correlated well with standard lab methods.



SCAN QR CODE FOR LINK



MEASUREMENT OF pH IN PLANT TISSUE



An optimal pH value of 6.4 in plant tissue will encourage healthy growth and prevent insects and diseases attacking the plant. To measure pH, squeeze the sap of mature leaves with garlic press and place the sap onto the sensor of LAQUAtwin pH meter.



SCAN QR CODE FOR LINK



CONDUCTIVITY AND ELEPHANT'S FOOT TESTING



Elephant's foot is a sweet pepper (*Capsicum annuum* L.) physiological disorder where the stem base swells below cotyledon level and wounds develop at the stem's epidermis base due to salt accumulation. LAQUAtwin conductivity meters can measure soil conductivity to help farmers select optimal land for sweet pepper cultivation.



SCAN QR CODE FOR LINK



SOIL pH AND NUTRIENT AVAILABILITY



The desirable soil pH range for optimum plant growth varies among crops. Generally, soil pH 6.0-7.5 is acceptable for most plants as most nutrients become available in this pH range. Soil pH can be determined by mixing soil sample with water and then measuring the resulting aqueous solution.



SCAN QR CODE FOR LINK



SOIL NITRATE MEASUREMENT FOR DETERMINATION OF PLANT-AVAILABLE NITROGEN



Nitrate concentration in soil is a good indicator of available nitrogen to plants. The required soil nitrate-nitrogen (NO₃-N) for specific crops varies from crop to crop but in general, a concentration range of 10-50 mg/kg is desired.



SCAN QR CODE FOR LINK



SOIL SALINITY MEASUREMENT IN ALMOND ORCHARD



Crops have different levels of tolerance to salinity. Testing soil salinity is the best way to check soil condition in the orchard before salt damage occurs. The $EC_{1:5}$ test is used to estimate soil salinity (EC_e). The soil salinity threshold value for almond is 1.5 mS/cm.



IMPACT OF SOIL SALINITY ON SUGAR CANE YIELD



Soil salinity adversely affects the growth of sugar cane crops. To help optimize sugar cane yield, check the sodium content in soil by mixing it with water in 1:5 ratio and measuring the resulting solution with LAQUAtwin sodium ion meter.



MEASUREMENT OF CALCIUM IN SOIL



Calcium is one of the essential nutrients taken up by plants from soil for cell wall development. To measure calcium concentration in soil, extraction with 1M ammonium acetate and filtration should be performed prior to placing the filtrate onto the flat sensor of LAQUAtwin calcium ion meter.



RAPID IN-FIELD DETERMINATION OF NITROGEN IN ONIONS



Fresh root sap analysis with LAQUAtwin nitrate ion meter offers cost-effective, rapid, and easy solution to determine nitrogen status in onion plants. The nitrate-nitrogen (NO_3-N) concentrations in onion vary at different growth stages. The acceptable root sap NO_3-N concentration range for 0.5 to 1.5-inch onion bulbs is 350 to 500 ppm.



NITRATE MEASUREMENT IN TURF GRASS



Nitrate concentration in grasses can be used as an indicator of soil nitrogen (N) availability for their growth. Research at the University of Connecticut suggests verdure sap nitrate-N concentrations at 200-300 ppm as the optimum level.



QUICK NUTRIENT ANALYSIS IN STRAWBERRY PRODUCTION



Regular monitoring of nutrient levels such as nitrate (NO_3^-), potassium (K^+) and calcium (Ca^{2+}) in plant petioles, soil solution, irrigation water and drain water produces not only good yield and fruit quality, but also reduces fertilizer cost and mitigates environmental hazards. LAQUAtwin pocket meters are the perfect tools for testing as they directly measure samples and provide results in just few seconds allowing growers to identify and correct any nutrient deficiency or excess immediately.



SCAN QR CODE FOR LINK



SCAN QR CODE FOR LINK



SCAN QR CODE FOR LINK



SCAN QR CODE FOR LINK



SCAN QR CODE FOR LINK



SCAN QR CODE FOR LINK



MEASUREMENT OF POTASSIUM IN SOIL



In laboratories, potassium in soil is extracted with 1M ammonium acetate and analyzed with Atomic Absorption (AA) or Inductivity Coupled Plasma-Optical Emission Spectrometry (ICP-OES). LAQUAtwin potassium ion meter showed values higher than those of ICP-OES. However, with 0.01M ammonium acetate extraction, good correlation ($r=0.981$, $r_2=0.962$) was obtained between ICP-OES and LAQUAtwin potassium ion meter.



POTASSIUM DETERMINATION IN PLANT TISSUE



Comparison of LAQUAtwin Potassium Ion Meter and ICP Spectrometry Trials revealed strong correlation (r values were 0.80 and 0.93 for 1st and 2nd trials, respectively) between the LAQUAtwin potassium ion meter readings and ICP results obtained from plant's fresh petiole sap and dried tissue, respectively. This suggests that LAQUAtwin K^+ meter is an appealing field method substitute for rapid determination of potassium concentration in plants.



MEASUREMENT OF POTASSIUM IN RICE



Potassium is one of the essential plant nutrients supplied via fertilizer in most irrigated rice fields. Extracting sap from the lower stem of plant rice and analysing it with LAQUAtwin potassium meter provide indication of the current potassium status and help farmers adjust the fertilizer application.



pH AND CONDUCTIVITY FOR TESTING ACRYLIC PAINT FILMS AND PAPER SUPPORTS AND FORMULATING AQUEOUS CLEANING SOLUTIONS



Isotonic aqueous cleaning solutions that match the pH and conductivity readings of acrylic paint films and paper supports obtained from agarose gel pellets have been shown to be effective in reducing or removing dirt, dust, active mold growth and associated stains, tide line stains, and discoloration.



AQUARIUM WATER TESTING



Testing aquarium water such as freshwater and saltwater (either natural or artificial seawater) with reliable instruments is necessary to create a clean and safe environment for your aquatic species. The LAQUAtwin pocket meters require only few drops of water and deliver the results in just few seconds.



pH MEASUREMENT IN THE ACIDIFICATION OF FERMENTED SAUSAGES



Lowering pH or increasing acidity of meat has become main hurdle against pathogenic bacteria in sausage making. pH is used in the course of fermentation process in order to produce microbiologically stable product that has a pH value of 5.3 or less.



SCAN QR CODE FOR LINK



SCAN QR CODE FOR LINK



SCAN QR CODE FOR LINK



SCAN QR CODE FOR LINK



SCAN QR CODE FOR LINK



SCAN QR CODE FOR LINK



pH OF BRINE FOR CANNED FOOD TESTING



For brine of canned acid foods, the equilibrium pH value must be 4.6 or below to inhibit the growth of *Clostridium botulinum*, the most heat resistant of the food pathogen microorganisms.



pH MEASUREMENT TO DETERMINE FRESHNESS OF MEAT PRODUCTS



Fresh meat must have a pH value in the range of 5.5 to 6.2 before selling to consumers. LAQUAtwin pH meter provides a simple and cost effective way to check the freshness of meat in the local markets.



pH MEASUREMENT TO DETERMINE ACIDIFICATION OF SUSHI RICE



The rice used for sushi must be acidified with acetic acid (vinegar) to pH less than 4.6 to inhibit the growth of pathogenic bacteria. To measure pH, simply place a sample of rice mixture onto the flat sensor of LAQUAtwin pH meter.



MEASUREMENT OF CALCIUM IN MILK AND MILK BEVERAGES



Determining the calcium content of milk and milk beverages helps consumers accurately gauge their calcium intake. Unlike atomic absorption spectroscopy (AAS) and inductively coupled plasma atomic emission spectroscopy (ICP), the LAQUAtwin calcium ion meter offers a simpler method of measuring calcium ion-ionizing protein-bound calcium in sample using acid before analysis.



MEASUREMENT OF SODIUM IN ATHLETE'S SWEAT



Determining the sodium concentration in sweat and replacing that with proper electrolyte intake prevent fluid and electrolyte imbalances. Sweat can be easily extracted from sterile patches applied on skin and tested with LAQUAtwin sodium ion meter. According to Gatorade Sports Science Institute, the sodium results obtained with HORIBA falls within 15.4 mEq/L 95% of the time.



pH OF CEMENT FOR FLOOR INSTALLATION TESTING



Fresh concrete is usually very alkaline, above pH 11. When the alkalinity in a concrete subfloor is high, it can stop the floor covering adhesive from bonding properly to the concrete. Australian Standard 1884 for resilient flooring installation states the pH level of the concrete surface should be between 9 and 10 before the flooring can be installed.



SCAN QR CODE FOR LINK



SCAN QR CODE FOR LINK



SCAN QR CODE FOR LINK



SCAN QR CODE FOR LINK



SCAN QR CODE FOR LINK



SCAN QR CODE FOR LINK



pH MEASUREMENT OF PICKLED FRUITS AND VEGETABLES



Pickling is a process of preserving fruits and vegetables in brine, oil, water or vinegar. The Australia New Zealand Food Standard Code 2.3.1 requires the preserved fruits and vegetables to have a pH not greater than 4.6 to prevent botulism.



DETERMINATION OF SODIUM CONTENT IN FOOD SAMPLES



Foods contain varying amounts of salt (NaCl), which has 40% sodium. Determining the sodium content in foods accurately reduces the health risks associated with it. The American Heart Association recommends consumption of less than 1500 mg/day sodium for most American adults, which is the level with the greatest effect on blood pressure.



SODIUM VALUE CHECK FOR CANNED FOOD



There is a growing concern on canned foods with large sodium content as excessive intake of sodium can cause high blood pressure and hypertension. To check the sodium content in canned food, dilute a sample with DI water in 1:5 ratio, then place the resulting solution onto the LAQUAtwin sodium ion meter.



DETERMINATION OF POTASSIUM IN SEA WATER



Seawater has high ionic strength. To eliminate matrix effect in measuring the potassium (K⁺) concentration, the standard solutions made with the same background as the seawater sample are recommended for calibration. The result of measurement using the LAQUAtwin Potassium Ion meter is within ±10% of typical seawater concentration.



RESIDUAL SODIUM CHECK DURING CLEAN-IN-PLACE PROCESS



Caustic soda or sodium hydroxide (NaOH) is the chemical commonly used in alkaline cleaning solution for clean-in-place (CIP) in process plants. Measuring the sodium ion concentration on the water rinse or swab can indicate whether residual chemical has been removed properly from the process equipment.



MEASURING SALINITY OF WATER



Measuring the salinity or the dissolved salt content of water is important as aquatic organisms, livestock, and crops thrive at different salinity levels. Freshwater has a salinity value of less than 0.5 ppt while seawater has an average salinity of 35 ppt.



SCAN QR CODE FOR LINK



SCAN QR CODE FOR LINK



SCAN QR CODE FOR LINK



SCAN QR CODE FOR LINK



SCAN QR CODE FOR LINK



SCAN QR CODE FOR LINK

Scan for More Application Notes





Meter Specifications



Model#	pH-11				pH-22				pH-33				ORP-11		
Parameters	 		 		  		 								
Features	   	   	   	  											
Part No.	3999960122				3999960123				3999960124				3200965260		
Measurement Principle	Glass Electrode										ORP Electrode				
Min. Sample	0.1 ml (0.05 ml with Sampling Sheet B)										0.3ml (0.05ml with Sampling Sheet B)				
pH Range / Resolution	0.0 to 14.0 pH / 0.1 pH				0.00 to 14.00 pH / 0.01 pH						—				
mV Range / Resolution	-650 to 650 mV / 1 mV										-1000 to 1000 mV / 1 mV				
Accuracy	± 0.1 pH				± 0.01 pH						± 2 mV				
Max. Calibration Points	2				3				5				1		
Calibration Curves	USA: 1.68, 4.01, 7.00, 10.01 & 12.46 NIST: 1.68, 4.01, 6.86, 9.18 & 12.46										225 mV				
Temperature Display / Resolution	—						0 to 50.0 °C / 0.1 °C								
Functions	• Automatic Buffer Recognition										• ORP and Eh Measurements • Automatic Standard Recognition • Auto / Custom Calibration Value				
	• Temperature Compensation • Temperature Calibration* • Auto Hold / Auto Stable • Automatic Power Off (30 mins)						• Low Battery Indicator • Rated IP67 Water / Dust Proof • Replaceable Sensor								
Display	Custom (Monochrome) Digital LCD with Backlight														
Operating Temperature / Humidity	5 to 40 °C / 85% or less in relative humidity (no condensation)														
Battery Life	Approx. 400 hrs. continuous use without backlight														
Materials	ABS epoxy body / flat glass sensor										ABS epoxy body / platinum disk sensor				
Dimensions	164 x 29 x 20 mm (excluding projections)														
Mass	Approx. 50g (excluding batteries)														
Accessories included	• pH 7.00 & 4.01 Buffers (14 ml each)										• 225 mV ORP Standard (14 ml) • Abrasive Cotton Swab • Sampling Sheet B (5 pcs)				
	• Dropper • Instruction & Quick Manuals • Storage Case														


*Applicable for models with temperature display #Requires 2 x CR2032 batteries (not included)



Model#	4EC-11				4EC-22				4EC-33				4ECSalt-11			
Parameters					 				  				 			
Features	   	   	   	   												
Part No.	3201077522				3201077523				3201077524				3201077528			
Measurement Principle	4 Electrode															
Min. Sample	0.12 ml															
Measurement Range / Resolution	Conductivity 0 to 199 $\mu\text{S}/\text{cm}$ (1 $\mu\text{S}/\text{cm}$) 200 to 1999 $\mu\text{S}/\text{cm}$ (1 $\mu\text{S}/\text{cm}$) 2.00 to 19.99 mS/cm (0.01 mS/cm)				Conductivity 0 to 199 $\mu\text{S}/\text{cm}$ (1 $\mu\text{S}/\text{cm}$) 200 to 1999 $\mu\text{S}/\text{cm}$ (1 $\mu\text{S}/\text{cm}$) 2.00 to 19.99 mS/cm (0.01 mS/cm) 20.0 to 199.9 mS/cm (0.1 mS/cm)				TDS 0.0 to 99.9 ppm (0.1 ppm) 100 to 999 ppm (1 ppm) 1000 to 9990 ppm (10 ppm)				Salinity 0.0 ppt to 100.0 ppt [†] : 0.1 ppt 0.00% to 10.00%: 0.01%			
	—				—				—				—			
Accuracy	$\pm 2\%$ full scale (for each range)				$\pm 2\%$ full scale (0 to 19.99 mS/cm) $\pm 5\%$ full scale (20.0 to 199.9 mS/cm)				$\pm 2\%$ full scale (0.0 to 9.9 ppt) $\pm 4\%$ full scale (10.0 to 100.0 ppt)							
Max. Calibration Points	3				4				2							
Calibration Curves	84 $\mu\text{S}/\text{cm}$, 1413 $\mu\text{S}/\text{cm}$, 12.88 mS/cm				84 $\mu\text{S}/\text{cm}$, 1413 $\mu\text{S}/\text{cm}$, 12.88 mS/cm, 111.8 mS/cm				TDS Factor (0.4 to 1.0) / EN 27888 / 442 / NaCl				NaCl / Sea water			
	—				—				—				—			
Temperature Display / Resolution	—				0 to 50.0 $^{\circ}\text{C}$ (0.1 $^{\circ}\text{C}$)											
Functions	- Automatic Range - Automatic Standard Recognition - Temperature Compensation (2%/$^{\circ}\text{C}$ fixed)				- Temperature Calibration* - Auto Hold / Auto Stable - Automatic Power Off (30 mins)				- Low Battery Indicator - IP67 Water / Dust Proof - Replaceable Sensor							
Display	Custom (Monochrome) Digital LCD with Backlight															
Operating Temperature/ Humidity	5 to 40 $^{\circ}\text{C}$ / 85% or less in relative humidity (no condensation)															
Battery Life	Approx. 400 hrs. continuous use without backlight															
Materials	ABS epoxy body / carbon sensor															
Dimensions	164 x 29 x 20 mm (excluding projections)															
Mass	Approx. 45g															
Accessories included	1413 $\mu\text{S}/\text{cm}$ & 12.88 mS/cm Conductivity Standard Solutions (14ml each) 5 ppt (0.5%) and 50 ppt (5%) NaCl Standard Solutions															
	- Conditioning Solution (4 ml) - Dropper - Instruction & Quick Manuals - Storage Case															

*Applicable for models with temperature display ^ppt = parts per thousand = g/L #Requires 2 x CR2032 batteries (not included)


TDS CALIBRATION CURVES		
APPLICATION	KEY CHEMICAL SPECIES	TDS SELECTION
Aquaculture, pickling	NaCl	NaCl
Boiler water, HVAC	Na ₂ SO ₄ , NaHCO ₃ , NaCl	442
Environmental	EN standard for environmental water	EN 27888
General application	KCl	TDS Factor Linear Default: 0.5 Selectable: 0.4 to 1.0

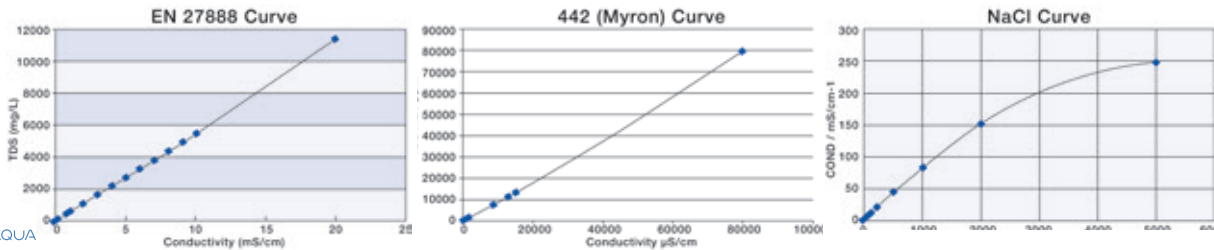

Model#	NO3-11	Na-11	K-11	Ca-11	F-11
Parameters	NO ₃ ⁻ Temp	Na ⁺ Temp	K ⁺ Temp	Ca ²⁺ Temp	F ⁻ Temp
Features	WATER PROOF MICRO VOLUME 2 PT CAL				
Part No.	3200689162	3200689159	3200689160	3200689161	3200934412
Measurement Principle	Ion Selective Electrode				
Min. Sample	0.3 ml (0.05 ml with Sampling Sheet B)				0.3ml (0.1ml with Sampling Sheet B)
Measurement Range	NO ₃ ⁻ : 6 to 9900 ppm (mg/L) (0.1 to 160 mmol/L) NO ₃ -N: 1.4 to 2200 ppm (mg/L)	2 to 9900 ppm (mg/L) (0.1 to 430 mmol/L)	4 to 9900 ppm (mg/L) (0.1 to 250 mmol/L) 2 to 5000 kg/10a (soil/water ratio 1:5)	4 to 9900 ppm (mg/L) (0.1 to 250 mmol/L)	0.1 to 990 ppm (mg/L)
Resolution	0 to 99 ppm: 1 ppm (mg/L) 100 to 990 ppm: 10 ppm (mg/L) 1000 to 9900 ppm: 100 ppm (mg/L)				0.1 to 9.9 ppm: 0.1 ppm 10 to 99 ppm: 1 ppm 100 to 990 ppm: 10 ppm
Accuracy	$\pm 10\%$ of actual value			$\pm 20\%$ of actual value	$\pm 2\%$ of actual value
Calibration Points	Up to 2				
Temperature Display / Resolution	0 to 50.0 $^{\circ}\text{C}$ / 0.1 $^{\circ}\text{C}$				
Functions	- Auto Standard Recognition - Changeable High and Low Calibration Values - Multiplying Compensation (0.01 to 9.90) - Temperature Calibration - Auto Hold / Auto Stable Measurement - Temperature Compensation - Automatic Power Off (30 mins) - Low Battery Indicator - Rated IP67 Dust/Waterproof - Replaceable Sensor				
Display	Custom (Monochrome) Digital LCD with Backlight				
Operating Temperature / Humidity	5 to 40 $^{\circ}\text{C}$ / 85% or less in relative humidity (no condensation)				
Battery Life	Approx. 400 hours in continuous use without backlight				
Materials	ABS epoxy body / PVC sensor				ABS epoxy body / LaF ₃ crystal sensor
Dimensions	164 x 29 x 20 mm (excluding projections)				
Mass	Approx. 50g (excluding batteries)				
Accessories included	150 & 2000 ppm Standard Solutions (14 ml each) - Dropper - Sampling Sheet B (5pcs) - Instruction & Quick Manuals - Storage Case 1 & 10 ppm Fluoride Standards (14 ml each) - TISAB (14 ml) 5 ml Beaker - Syringe				

#Requires 2 x CR2032 batteries (not included)

Correlation Between LAQUAtwin Measurement Data And Ion Chromatography

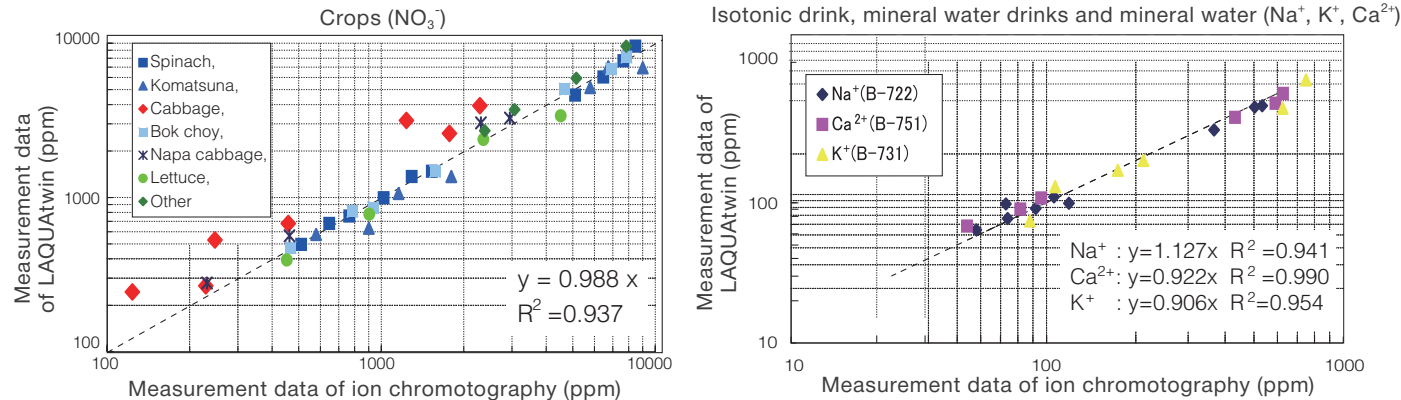

*When measuring Ca²⁺, samples are pretreated in order to match the conditions of the ion chromatography.

Accessories & Solutions

LAQUAtwin Replacement Sensors

Part No.	Model	Description
3200459834	S010	pH Sensor (for pH-11, pH-22 & pH-33)
3200459866	S021	Salt Sensor (for Salt-22)
3200459867	S022	Sodium Ion Sensor (for Na-11)
3200459868	S030	Potassium Ion Sensor (for K-11)
3200459870	S040	Nitrate Ion Sensor (for NO3-11, NO3-11C & NO3-11S)
3200459869	S050	Calcium Ion Sensor (for Ca-11)
3200459672	S070	Conductivity Sensor (for EC-11, EC-22 & EC-33)
3201079162	S073-4EC	Conductivity Sensor (for 4EC-11, 4EC-22 & 4EC-33)
3200597237	S071	Salt EC Sensor (for Salt-11)
3201079163	S074-4EC	Salt EC Sensor (for 4ECSalt-11)
3200934450	S060-F	Fluoride Ion Sensor (for F-11)
3200997083	S080-ORP	ORP Sensor (for ORP-11)



LAQUAtwin Replacement Sensors

LAQUAtwin Standard Solutions (6 x 14ml bottles per pack)

Part No.	Model	Description
3999960108	514-4	pH 4.01 Buffer
3200691954	514-686	pH 6.86 Buffer
3999960109	514-7	pH 7.00 Buffer
3999960110	514-22	1413 µS/cm Conductivity Standard Solution
3999960111	514-23	12.9 Conductivity Standard Solution
3999960112	514-05	0.5% NaCl Standard Solution
3999960113	514-50	5.0% NaCl Standard Solution
3999960114	514-20	Conditioning Solution (For EC-11, EC-22, EC-33 & Salt-11)
3201081522	514-4EC-CON	Conditioning Solution (For 4EC-11, 4EC-22, 4EC-33 & 4ECSalt-11)
3200457723	Y022H	2000ppm Sodium Ion Standard Solution
3200457724	Y022L	150ppm Sodium Ion Standard Solution
3200457719	Y031H	2000ppm Potassium Ion Standard Solution



pH Buffers



Conductivity Standard Solutions



NaCl Standard Solutions



Conditioning Solutions

3200457720	Y031L	150ppm Potassium Ion Standard Solution
3200053433	Y041	5000ppm Nitrate Ion Standard Solution
3200053514	Y042	300ppm Nitrate Ion Standard Solution
3200053532	Y043	2000ppm Nitrate Ion Standard Solution
3200053535	Y044	30ppm Nitrate Ion Standard Solution
3200053536	Y045	150ppm Nitrate Ion Standard Solution
3200457727	Y051H	2000ppm Calcium Ion Standard Solution
3200457728	Y051L	150ppm Calcium Ion Standard Solution
3200991628	514-F-1	1ppm Fluoride Ion Standard Solution
3200991630	514-F-10	10ppm Fluoride Ion Standard Solution
3200991632	514-F-TISAB	TISAB Solution
3200997084	514-ORP-225	225 mV ORP Standard Solution



Sodium Ion Standard Solutions



Potassium Ion Standard Solutions



Nitrate Ion Standard Solutions



Calcium Ion Standard Solutions



Fluoride Ion Standard Solutions



ORP Standard Solution



Sampling Sheet B



Sampling Sheet Holder

LAQUAtwin Accessories

Part No.	Model	Description
3200053858	Y046	Sampling Sheet B (100pcs) for minute samples (≥ 0.05ml)
3200459736	Y048	Sampling Sheet Holder (use with sampling sheet B for samples with particulates)



With over 70 years of engineering excellence, HORIBA's diverse range of water quality analyzers and electrodes are ideal for everyday laboratory needs through to the most demanding of applications. Discover more on our website for a wealth of useful information and water quality measurement tips to help you obtain the best results in your work.



www.horiba-laqua.com

Explore our collection of brochures.



LAQUA Water Quality Catalogue



LAQUA Electrodes & Accessories



LAQUA 2000 Series Benchtop Meters



LAQUA WQ-300 Series Smart Handheld Meters



LAQUA Benchtop Color Touchscreen Water Quality Meters



LAQUA 200 Series Handheld Water Quality Meters

Check out our application notes.



Available Online

Subscribe to our Youtube channel for product insights and demos.



Contact us today for water quality measurement solutions—your needs, our solutions.

ASIA PACIFIC

HORIBA Instruments (Singapore) Pte Ltd
 163 Kallang Way, #08-14,
 Mapletree Hi-Tech Park @ Kallang Way,
 Singapore 349256
 (65) 6745-8300
laqua@horiba.com

EUROPE, MIDDLE EAST & AFRICA

HORIBA UK Limited
 Kyoto Close, Moulton Park,
 Northampton NN3 6FL UK
 +44 1604 542 500
waterquality@horiba.com

AMERICAS

HORIBA Instruments Incorporated
 9755 Research Drive, Irvine,
 California 92618 USA
 +1 800 446 7422
labinfo@horiba.com



HORIBA Group is certified Quality Management System ISO9001, Environmental Management System ISO14001, and Occupational Health and Safety Management System ISO45001 and operate as Integrated Management System (IMS).



- Catalog contents may change without prior notice or any subsequent liability to this company.
- Product colors may vary due to printing.
- Reproduction of the catalog is prohibited.

- All brands and names are trademarks of their respective companies.
- Windows is a registered trademark of Microsoft Corporation in the United States and other countries.

Brochure PBT-04-2026A